



National Institute for Occupational Safety and Health
National Personal Protective Technology Laboratory
P.O. Box 18070
Pittsburgh, PA 15236

| | | | |
|-----------------------------------|---------|---------------|---------------------|
| Procedure No. STP-00001-PSDB-0004 | | Revision: 3.0 | Date: 28 March 2012 |
| Level 1 | Level 2 | Level 3 | Level 4 |

**STANDARD TESTING PROCEDURE (STP) TO CONDUCT MAN TEST 4 FOR
CLOSED-CIRCUIT ESCAPE RESPIRATORS (CCER) TO BE USED IN
UNDERGROUND COAL MINES**

1. PURPOSE

- 1.1. This test establishes the procedures for ensuring that the level of protection provided by the Man Test 4 requirements on Closed-Circuit Escape Respirators (CCER) submitted for Approval, Extension of Approval, or examined during Certified Product Audits, meet the minimum certification standards set forth in Section 84.304(a) (5) of Subpart O—Closed Circuit Escape Respirators updated requirements to 42 CFR, Part 84, Volume 60, Number 110, June 8, 1995 as published in Federal Register / Vol. 77, No. 46 / Thursday, March 8, 2012 / Rules and Regulations pp. 14168-14197.

2. GENERAL

- 2.1. This STP describes the Man Test 4 for Closed-Circuit Escape Respirator test in sufficient detail that a person knowledgeable in the appropriate technical field can assemble the appropriate equipment, conduct the test, and determine whether or not the product passes the test.

3. EQUIPMENT/MATERIALS

- 3.1. The list of necessary test equipment and materials follows:

- 3.1.1. One B-D Yale (2317 100YL) 100cc (Becton, Dickson and Co.) syringe "Luer-Lok", Becton Dickson & Company, Rutherford, NJ, or equivalent.

- 3.1.2. Doric Series 400A Digital Trendicator, Doric Scientific Division, Emerson Electric Company, 3883 Ruffin Road, San Diego, CA 92123 or equivalent.
- 3.1.3. Gould Stratham Transducer Readout, Model SC1012, Gould, Inc., 2230 Stratham Blvd., Oxnard, CA 93030 or equivalent.
- 3.1.4. Temperature Compensated Strain Sensitive Resistance wire-type transducer (Stratham Instruments) Pressure range +0.5 psig or equivalent.
- 3.1.5. Electric timer, calibrated to 100ths of a minute (Precision Scientific Co.) or equivalent.
- 3.1.6. Multiple outlet box with 6 receptacles or equivalent.
- 3.1.7. Timer/stopwatch to hand carry or equivalent.
- 3.1.8. Beckman LB-2 (digital readout) with positive/negative mode and positive and negative Peak Detectors, heated sample inlet and other accessories desired, Beckman LB-2 Medical Gas Analyzer available from Beckman Instruments, Inc., Electronic Instruments Division, 3900 River Road, Schiller Park, Illinois 60176 or equivalent.
- 3.1.9. Beckman medical Gas Analyzer – OM-11 (oxygen) or equivalent.
- 3.1.10. Oxygen - U.S.P or equivalent.
- 3.1.11. Carbon dioxide - calibration gas, 4-5%, 1-2%, 3-4% Matheson Scientific Company, E. Rutherford, NJ or equivalent.
- 3.1.12. Carbon dioxide calibration curve or equivalent.
- 3.1.13. Fifty-pound sack or equivalent.
- 3.1.14. Forty-five pound pipe weight or equivalent.
- 3.1.15. Forty-five pound weight pulling machine (U.S. BOM) or equivalent.
- 3.1.16. Knee pads or equivalent.
- 3.1.17. Matheson Gas Products Model # 8320 carbon dioxide regulator, East Rutherford, NJ or equivalent.
- 3.1.18. Dwyer Slant Manometer, F. W. Dwyer Manufacturing Co., Michigan City, Indiana (Fisher Scientific Company) or equivalent.

| | | | |
|-----------------------------------|---------------|---------------------|--------------|
| Procedure No. STP-00001-PSDB-0004 | Revision: 3.0 | Date: 28 March 2012 | Page 3 of 20 |
|-----------------------------------|---------------|---------------------|--------------|

- 3.1.19. Model 18-49B Horizontal Treadmill, 0-6 MPH, Quinton Instruments, 3051 44th Avenue, West Seattle, Washington 98199 or equivalent.
- 3.1.20. Model 24-90 Ladderwalk 0-130 feet/minute, Quinton Instruments, 3051 44th Avenue, West Seattle, Washington 98199 or equivalent.
- 3.1.21. Two test subjects meeting requirements of the NIOSH Human Subject Review Board (HSRB) approved Protocol. Refer to “Protocol for tests with human subjects of closed-circuit breathing apparatus in certification, quality assurance, and development” HSRB 12-NPPTL-04 for the proper consent form and complete details on the use of human test subjects in respirator certification testing.
- 3.1.22. An automated external defibrillator (AED) at the test scene.

4. TESTING REQUIREMENTS AND CONDITIONS

- 4.1. Prior to beginning any testing, all measuring equipment to be used must have been calibrated in accordance with the manufacturer's calibration procedure and schedule. At a minimum, all measuring equipment utilized for this testing must have been calibrated within the preceding 12 months using a method traceable to the National Institute of Standards and Technology (NIST).
- 4.2. Any laboratory using this procedure to supply certification test data to NPPTL will be subject to the provisions of the NPPTL Supplier Qualification Program (SQP). This program is based on the tenets of ISO/IEC 17025, the NIOSH Manual of Analytical Methods and other NIOSH guidelines. An initial complete quality system audit and follow on audits are requirements of the Program. Additional details of the Program and its requirements can be obtained directly from NPPTL.
- 4.3. Normal laboratory safety practices must be observed. These include safety precautions given in the current *NIOSH-Pittsburgh Health and Safety Manual*, Job Hazard Analysis (JHA), work instruction documents and test equipment manufacturer recommended practices.
- 4.4. Refer to HSRB 12-NPPTL-04, “Protocol for tests with human subjects of closed-circuit breathing apparatus in certification, quality assurance, and development” for the proper consent form and complete details on the use of human test subjects in closed-circuit escape respirator certification testing.

| | | | |
|-----------------------------------|---------------|---------------------|--------------|
| Procedure No. STP-00001-PSDB-0004 | Revision: 3.0 | Date: 28 March 2012 | Page 4 of 20 |
|-----------------------------------|---------------|---------------------|--------------|

5. PROCEDURE

Note: Reference Section 3 for equipment, model numbers and manufacturers. For calibration purposes use those described in the manufacturer's operation and maintenance manuals.

5.1. Use the test operating procedure as follows:

5.1.1. The man tests are conducted in duplicate in accordance with the specific duration test schedule corresponding to the service time approval requested by the manufacturer.

5.1.2. During the sampling periods the following parameters are monitored:

Closed Circuit

- a) breathing resistance
- b) gauge pressure
- c) subject pulse rate
- d) subject respiration rate
- e) oxygen in inhalation tube
- f) carbon dioxide in inhalation tube
- g) temperature (mask and ambient)

5.1.3. Prior to tests the oxygen and carbon dioxide analyzers must be calibrated with the proper calibration gas (see 3.1.10. and 3.1.11.) and the resistance instrument must be calibrated with a slant manometer.

5.1.4. All tests require the services of a physician, and a crash cart with current dated drugs and equipment at the test scene.

5.1.5. Test subjects are used for evaluation of a CCER for use in coal mines. Refer to HSRB 12-NPPTL-04 "Protocol for tests with human subjects of closed-circuit breathing apparatus in certification, quality assurance, and development".

TEST SUBJECTS CHECK LIST

Test Subject
1-week Notice

MSHA Personnel
2-week Notice

1. _____ Arrange Test Dates
2. _____ Confirm with Letter

1. _____ Arrange Test Dates

(A) Confirm M.D. Availability

1. _____ on planned test dates
2. _____ call Manufacturer (test dates)
3. _____ Test Prep. Sheet and Man Test Sheet

(B) Subject Arrival

1. _____ Orientation (Protocol Activity Sheets)
2. _____ Subject Reads Protocol
3. _____ Subject Signs NIOSH IRB protocol Consent Form
4. _____ Orientation on Exercise Equipment
5. _____ Explain Respirator Operation and Donning

(C) _____ Conduct Tests

(D) _____ Meet and Review Comments

(E) _____ Pay Participants

(F) _____ Write Letter of Appreciation

OUTLINE (TEST SUBJECT SAFEGUARDS)

- I. Presubmission - Manufacturer performs tests, as required by Part 84, on their apparatus to demonstrate conformance to regulations.
- II. Apparatus Testing
 - (A) Laboratory tests performed
 - 1. Must meet all applicable performance requirements
 - 2. Must be of safe design
 - (B) Modifications must be made by manufacturer and apparatus retested for performance
- III. Pre-subject preparation
 - (A.) All testing personnel have current CPR (including AED) training and certificates
 - (B.) Notices of subject tests are sent to appropriate NIOSH personnel including:
 - 1. Staff involved in testing
 - 2. Physician
 - 3. Front desk guard
 - 4. Administrative Officer
- IV. Pre-test preparation
 - (A.) Physician and Team Leader have pagers for immediate notification of:
 - 1. Emergency
 - 2. Problems
 - (B.) Test subject receives a physical examination by Physician
 - 1. Must meet all physical requirements
 - 2. Must be referred by Physician as satisfactory
 - (C.) Test subject orientation
 - 2. If new, tries out work exercise equipment
 - 3. Is given information regarding test apparatus
 - 4. Reads and signs HSRB document to safeguard subject
 - 5. Reads protocol (test)
 - 6. Given opportunity to ask questions
 - 7. Is told that he is permitted to stop test anytime for any reason he feels justified
 - 8. Asked if he is prepared to begin test

V. Testing

- A. Two personnel present during tests
- B. Crash cart present with current drugs and calibrated defibrillator
- C. Subject monitored for oxygen concentration. CO₂ levels, resistance, temperatures, respirations, pulse rate (test stopped if regulations levels are exceeded), and blood oxygen saturation (pulse oximetry).

BEFORE-EACH-MAN-TEST CHECK LIST

1. Suction Machine
2. Batteries and Bulbs in Laryngoscope
3. Batteries and Bulbs in Flashlight
4. Dates on Medication
5. Check O₂ Cylinder
6. Unlock Crash Cart

| <u>Date Checked</u> | <u>Signature</u> | <u>Task Number</u> | <u>Unit</u> | <u>Man Test No.</u> |
|---------------------|------------------|--------------------|-------------|---------------------|
| _____ | _____ | _____ | _____ | _____ |
| _____ | _____ | _____ | _____ | _____ |
| _____ | _____ | _____ | _____ | _____ |

5.2. Data Analysis

5.2.1. All sample values must be within the regulations requirements. Other factors are also evaluated during the tests, such as; strap length, position and adjustments; comfort; weight; profile; total performance. Expert test subjects give test feedback and opinions for the SCBA evaluated and are geared towards:

5.2.2. General comments

5.2.3. Specific comments per intended application.

Note: This test will be done on a minimum of two respirators, or more if additional testing is required (42 CFR, Part 84, Sections 84.12, 84.30, and 84.60.)

6. PASS/FAIL CRITERIA

6.1. The criterion for passing this test is set forth in 42 CFR, Part 84, Subpart G, Section 84.63(a)(c)(d), and Subpart H, Section 84.70, 84.79(a), 84.97, 84.99, 84.100, 84.103, Volume 60, Number 110, June 8, 1995.

6.2. This test establishes the standard procedure for ensuring that:

84.63 Test requirements; general.

(a) Each respirator and respirator component shall when tested by the applicant and by the Institute, meet the applicable requirements set forth in subparts H through L of this part.

(c) In addition to the minimum requirements set forth in subparts H through L of this part, the Institute reserves the right to require, as a further condition of approval, any additional requirements deemed necessary to establish the quality, effectiveness, and safety of any respirator used as protection against hazardous atmospheres.

(d) Where it is determined after receipt of an application that additional requirements will be required for approval, the Institute will notify the applicant in writing of these additional requirements, and necessary examinations, inspections, or tests, stating generally the reasons for such requirements, examinations, inspections, or tests.

84.79 Breathing gas; minimum requirements

(a)-1 Breathing gas used to supply apparatus shall be respirable and contain no less than 19.5 (dry atmosphere) volume percent of oxygen.

84.97 Test for carbon dioxide in inspired gas; closed-circuit apparatus; maximum allowable limits.

- (c) During the testing required by paragraphs (a) and (b) of this section, the concentration of carbon dioxide in inspired gas at the mouth will be continuously recorded, and the maximum average concentration during the inhalation portion of the breathing cycle shall not exceed the following limits:

| Where the service time is | Maximum allowable average concentration of carbon dioxide in inspired air percent by volume |
|-------------------------------|---|
| Not more than 30 minutes..... | 2.5 |
| 1 hour..... | 2.0 |
| 2 hour..... | 1.5 |
| 3 hour..... | 1.0 |
| 4 hour..... | 1.0 |

84.99 Man tests; testing conditions; general requirements.

- (a) The man tests described in Table 4 represent the workload performed in the mining, mineral, or allied industries by a person wearing the apparatus tested.
- (b) The apparatus tested will be worn by personnel trained in the use of self-contained breathing apparatus, and the wearer will, before participating in these tests, pass a physical examination conducted by a qualified physician.
- (c) All man tests will be conducted by the Institute.
- (d) The apparatus will be examined before each man test to ensure that it is in proper working order.
- (e) Breathing resistance will be measured within the facepiece or mouthpiece and the wearer's pulse and respiration rate will be recorded during each 2-minute sample period prescribed in tests 1, 2, 3, and 4.
- (f) Man tests 4 will be conducted in duplicate.
- (g) If man tests are not completed through no fault of the apparatus, the test will be repeated.

84.100 Man test 4; requirements.

Man test 4, set forth in Table 4 respectively, prescribe the duration and sequence of specific activities. These tests will be conducted to:

- (a) Familiarize the wearer with the apparatus during use;
- (b) Provide for a gradual increase in activity;
- (c) Evaluate the apparatus under different types of work and physical orientation; and
- (d) Provide information on the operating and breathing characteristics of the apparatus during actual use.

84.103 Man tests; performance requirements.

- (a) The apparatus shall satisfy the respiratory requirements of the wearer for the classified capacity (Cap 3 for one hour test duration).
- (b) Fogging of the eyepiece shall not obscure the wearer's vision, and the wearer shall not experience undue discomfort because of fit or other characteristics of the apparatus.
- (c) When the ambient temperature during testing is 24 degrees \pm 6 degrees C. (75 degrees \pm 10 degrees F.), the maximum temperature of inspired air recorded during man tests shall not exceed the following, after correction for deviation from 24 degrees C. (75 degrees F.):

| Where service life of apparatus is-- | Where percent relative humidity of inspired air is-- | Maximum permissible temperature of inspired air shall not exceed-- | |
|--------------------------------------|--|--|-----------------|
| | | | |
| 1/4 hour or less | 0-100 | 135 | 57 |
| 1/2 hour to 3/4 hour | 0-50 | 125 | 52 |
| | 50-100 | 110 ¹ | 43 ¹ |
| 1 to 2 hours | 0-50 | 115 | 46 |
| | 50-100 | 105 ¹ | 41 ¹ |
| 3 hours | 0-50 | 110 | 43 |
| | 50-100 | 100 ¹ | 38 ¹ |
| 4 hours | 0-50 | 105 | 41 |
| | 50-100 | 95 ¹ | 35 ¹ |

¹Where percent relative humidity is 50-100 and apparatus is designed for escape only, these maximum permissible temperatures will be increased by 5°C (10°F).

Tables to Subpart H of Part 84

Table 4-Duration and Sequence of Specific Activities for Test 4, in Minutes
[42 CFR part 84, subpart H]

| Activity | Service time- | | | | | | | | | |
|--|----------------------|-----------------------|-----------------------|-----------------------|-----------------------|-----------------------|-----------------------|------------------|------------------|------------------|
| | 3 minutes | 5 minutes | 10 minutes | 15 minutes | 30 minutes | 45 minutes | 1 hour | 2 hours | 3 hours | 4 hours |
| Sampling and readings | | | | 2 | 2 | 2 | 2 | (²) | (³) | (⁴) |
| Walks at 4.8 km. (3 miles) per hour | | | | 1 | 2 | 2 | 2 | | | |
| Climbs vertical treadmill 1 (or equivalent) | 1 | 1 | 1 | 1 | 1 | 1 | 1 | | | |
| Walks at 4.8 km. (3 miles) per hour | | 1 | 1 | 1 | 2 | 2 | 2 | | | |
| Pulls 20 kg. (45 pound) weight to 5 feet | | 30 times in 2 minutes | 30 times in 2 minutes | 30 times in 2 minutes | 60 times in 5 minutes | 60 times in 5 minutes | 60 times in 5 minutes | | | |
| Walks at 4.8 km. (3 miles) per hour | | | 1 | 1 | 1 | 2 | 3 | | | |
| Carries 23 kg. (50 pound) weight over overcast | | | | 1 time in 1 minute | 1 time in 1 minute | 2 times in 3 minutes | 4 times in 8 minutes | | | |
| Sampling and readings | | | 2 | | 2 | 2 | 2 | | | |
| Walks at 4.8 km. (3 miles) per hour | | | | 1 | 3 | 3 | 4 | | | |
| Runs at 9.7 km. (6 miles) per hour | | 1 | 1 | 1 | 1 | 1 | 1 | | | |
| Carries 23 kg. (50 pound) weight over overcast | | | 1 time in 1 minute | 1 time in 1 minute | 2 times in 3 minutes | 4 times in 6 minutes | 6 times in 9 minutes | | | |
| Pulls 20 kg (45 pound) weight to 5 feet | 15 times in 1 minute | | | 15 times in 1 minute | 60 times in 5 minutes | 30 times in 2 minutes | 36 times in 3 minutes | | | |
| Sampling and readings | | | | 2 | 2 | 2 | 2 | | | |
| Walks at 4.8 km. (3 miles) per hour | 1 | | 1 | | | 2 | 6 | | | |
| Pulls 20 kg. (45 pound) weight to 5 feet | | | | | | 60 times in 5 minutes | 60 times in 5 minutes | | | |
| Carries 20 kg. (45 pound) weight and walks at 4.8 km. (3 miles) per hour | | | | | | 3 | 3 | | | |
| Sampling and readings | | | | | | 2 | 2 | | | |

¹Treadmill shall be inclined 15° from vertical and operated at a speed of 30 cm. (1 foot) per second.

²Perform test No. 1 for 30-minute apparatus; then perform test No. 4 for 1-hour apparatus; then perform test No. 1 for 30-minute apparatus.

| | | | |
|-----------------------------------|---------------|---------------------|---------------|
| Procedure No. STP-00001-PSDB-0004 | Revision: 3.0 | Date: 28 March 2012 | Page 14 of 20 |
|-----------------------------------|---------------|---------------------|---------------|

³Perform test No. 1 for 1-hour apparatus; then perform test No. 4 for 1-hour apparatus; then perform test No. 1 for 1-hour apparatus.

⁴Perform test No. 1 for 1-hour apparatus; then perform test No. 4 for 1-hour apparatus; then perform test No. 1 for 1-hour apparatus twice (i.e., two one-hour tests).

7. RECORDS\TEST SHEETS

7.1. All test data will be recorded on the MAN TESTS, SELF-CONTAINED BREATHING APPARATUS test data sheet.

7.2. All videotapes and photographs of the actual test being performed, or of the tested equipment shall be maintained in the task file as part of the permanent record.

7.3. All equipment failing any portion of this test will be handled as follows:

7.3.1. If the failure occurs on a new certification application, or extension of approval application, send a test report to the RCT Leader and prepare the hardware for return to the manufacturer.

7.3.2. If the failure occurs on hardware examined under an Off-the-Shelf Audit the hardware will be examined by a technician and the RCT Leader for cause. All equipment failing any portion of this test may be sent to the manufacturer for examination and then returned to NIOSH. However, the hardware tested shall be held at the testing laboratory until authorized for release by the RCT Leader, or his designee, following the standard operating procedures outlined in Procedure for Scheduling, and Processing Post-Certification Product Audits, RB-SOP-0005-00.

MAN TESTS, SELF-CONTAINED BREATHING APPARATUS #4 - 4 HOUR

PROJECT NO: _____ DATE : _____

Subject: _____ Age : _____

Subject weight: Initial - _____ Final - _____

RESPIRATOR TYPE: 4 hour

Unit weight: Initial - _____ Final - _____

Observers: _____

Sampling Schedule

| Time/Min. | Gas Percent | Pulse | Resp. | Resistance | Temperature | Press |
|-----------|--------------------------------|-------|-------|------------|-------------|-------|
| _____ | CO ₂ O ₂ | bpm | rpm | inh. exh. | unit amb. | gauge |
| 0-2 | _____ | _____ | _____ | _____ | _____ | _____ |
| 20-22 | _____ | _____ | _____ | _____ | _____ | _____ |
| 40-42 | _____ | _____ | _____ | _____ | _____ | _____ |
| 58-62 | _____ | _____ | _____ | _____ | _____ | _____ |
| 83-85 | _____ | _____ | _____ | _____ | _____ | _____ |
| 102-104 | _____ | _____ | _____ | _____ | _____ | _____ |
| 118-122 | _____ | _____ | _____ | _____ | _____ | _____ |
| 140-142 | _____ | _____ | _____ | _____ | _____ | _____ |
| 160-162 | _____ | _____ | _____ | _____ | _____ | _____ |
| 178-182 | _____ | _____ | _____ | _____ | _____ | _____ |
| 200-202 | _____ | _____ | _____ | _____ | _____ | _____ |
| 220-222 | _____ | _____ | _____ | _____ | _____ | _____ |
| 238-240 | _____ | _____ | _____ | _____ | _____ | _____ |

Alarm - _____ min. at _____ psig.

Work Schedule

| <u>Time/Min.</u> | <u>Exercise</u> |
|------------------|-------------------------------|
| 0-2 | sample |
| 2-20 | walk - 3mph |
| 20-22 | sample |
| 22-40 | walk - 3mph |
| 40-42 | sample |
| 42-58 | walk - 3mph |
| 58-62 | sample |
| 62-64 | walk - 3mph |
| 64-65 | vertical |
| 65-67 | walk - 3mph |
| 67-72 | rope pull - 60x5min |
| 72-75 | walk - 3mph |
| 75-83 | overcast - 4x8min |
| 83-85 | sample |
| 85-89 | walk - 3mph |
| 89-90 | run - 6mph |
| 90-99 | overcast - 6x9min |
| 99-102 | rope pull - 36x3min |
| 102-104 | sample |
| 104-110 | walk - 3mph |
| 110-115 | rope pull - 60x6min |
| 115-118 | carry 45lb weight & walk 3mph |

Work Schedule (cont)

| <u>Time/Min.</u> | <u>Exercise</u> |
|------------------|-----------------|
| 118-122 | sample |
| 122-140 | walk - 3mph |
| 140-142 | sample |
| 142-160 | walk - 3mph |
| 160-162 | sample |
| 162-178 | walk - 3mph |
| 178-182 | sample |
| 182-200 | walk - 3mph |
| 200-202 | sample |
| 202-220 | walk - 3mph |
| 220-222 | sample |
| 222-238 | walk - 3mph |
| 238-240 | sample |

Comments :

Test Engineer: _____ PASS _____ FAIL _____

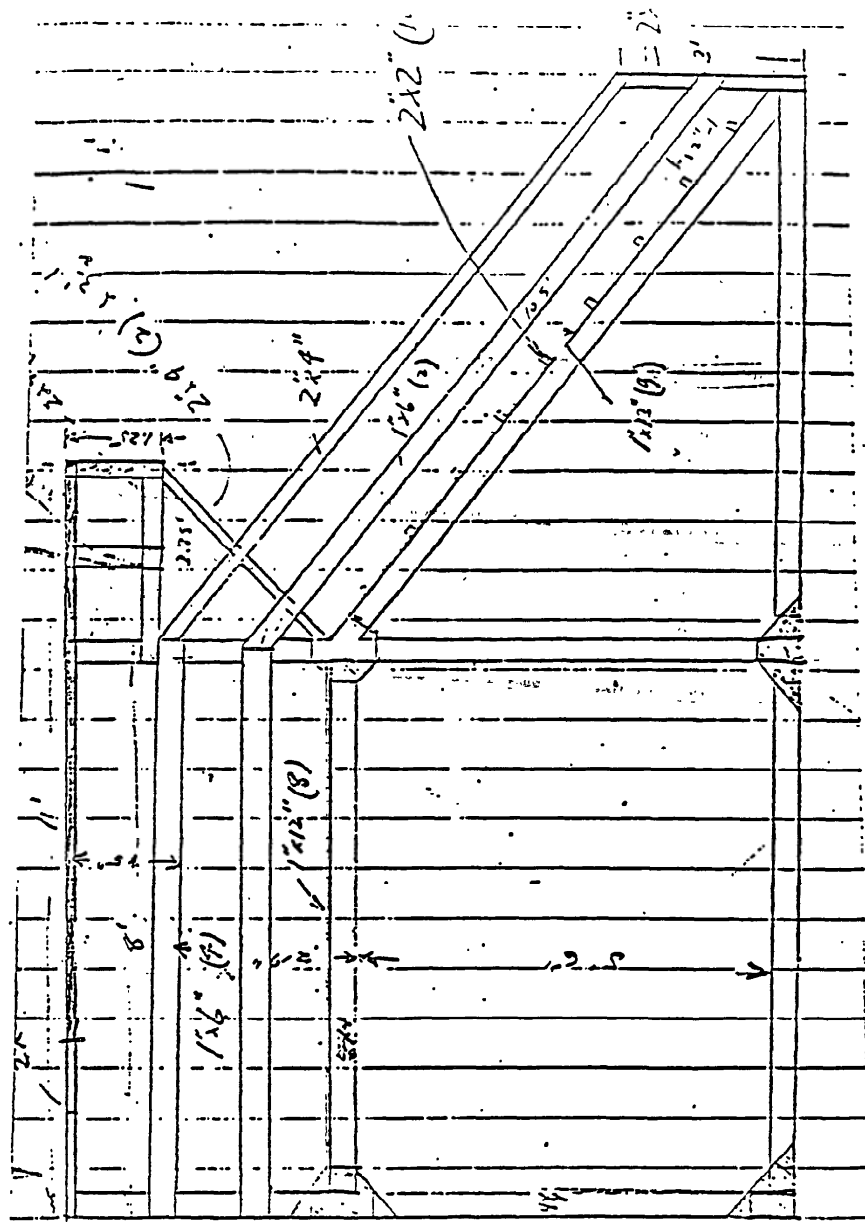


Figure 10

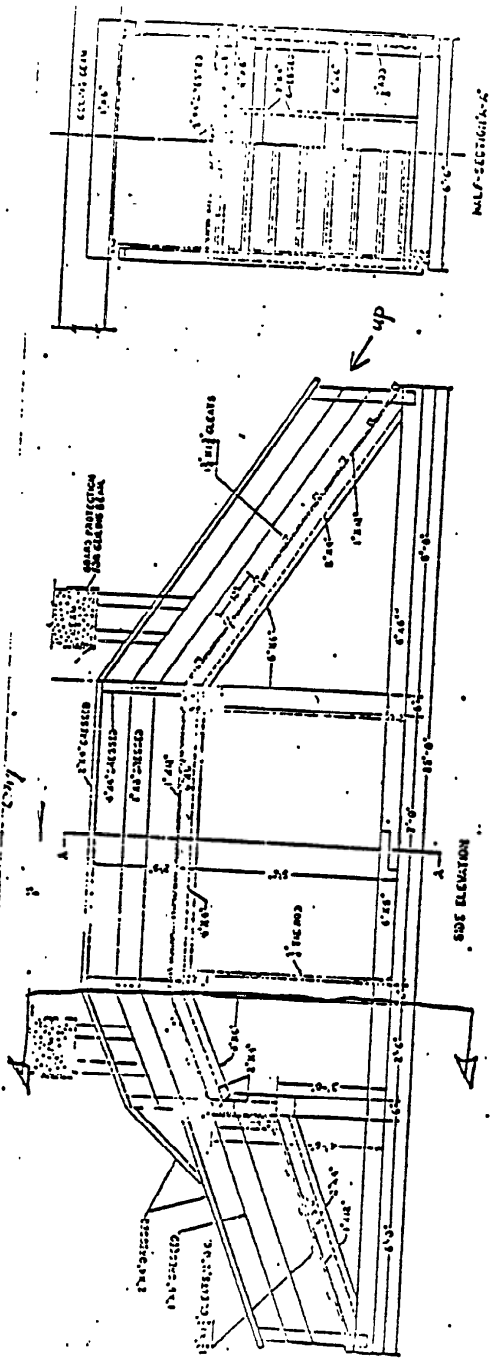


FIGURE 9—Overpass.

8. APPENDICES

INTENTIONALLY LEFT BLANK

9. REVISION HISTORY

| Revision | Date | Reason for Revision |
|-----------------|------------------|--|
| 00 | 07 October 2009 | Initial Record |
| 1.0 | 16 November 2011 | Administrative change – Document number changed |
| 2.0 | 20 February 2012 | Man Test 4 for CAP-3 Closed-circuit Escape Respirators (CCER) Standard Testing Procedure (STP) |
| 3.0 | 28 March 2012 | Administrative changes were made to include information from the release of the proposed rule. |